




POWERPRESS UNIT

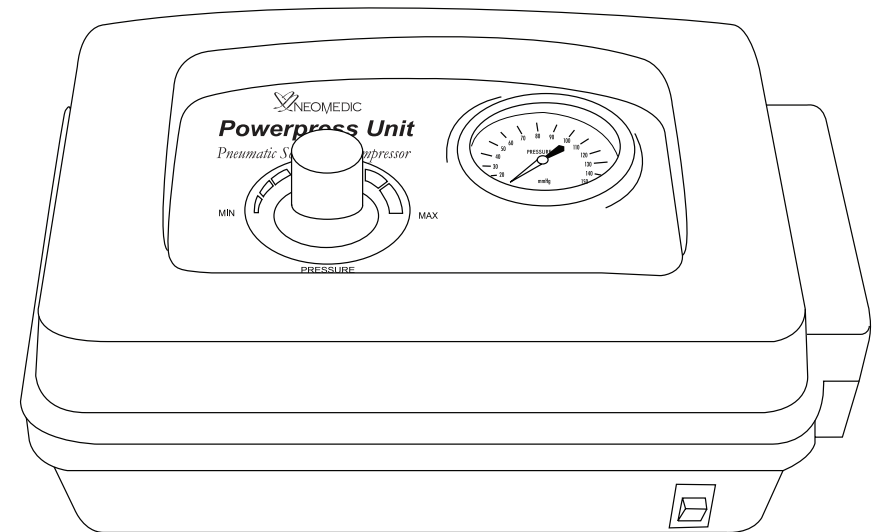

User Manual

Neomedic

9601 Owens mouth Ave. #8
Chatsworth, CA 91311

Toll Free: 866-990-1168

Tel: 818-998-1023

Fax: 818-998-0277

www.air1000.com

info@air1000.com

Pneumatic Sequential Compressor

Contents

1. Introduction -----	4
2. Clinical Application-----	5
3. Clinical Treatment Guide -----	6
4. Garment type & Size-----	7
5. Pump Description -----	8
6. Warranty -----	10
7. General Safety-----	10
8. Caution-----	10
9. Trouble Shooting-----	11
10. Technical Description-----	11

1. Introduction

The Powerpress Unit system consists of a pneumatic pump which is light and simple to use and a 4 chamber garment. It is suitable for home use.

The pump supplies air via connecting tubes to an inflatable garment allowing the application of controlled pressure to gently compress the limb. This action assists in increasing the return of blood, excess fluids, improves venous stasis and encourages the reabsorption of waste products.

Compression Cycle:

36sec inflation (9sec each chamber) / 24 sec deflation

Chamber 1 (Foot) = 36sec

Chamber 2 (Ankle) = 27sec

Chamber 3 (Calf) = 18sec

Chamber 4 (Thigh) = 9sec

Variable pressure output ranges from 30-160 mmHg. The segments within the garments are designed to prevent ridging and ensure high patient comfort and compliance.

** We would recommend that this manual is read thoroughly before proceeding with treatment. Please also refer to clinical guidelines and contraindications.

2. Clinical Application

Intermittent Compression Therapy

A thorough assessment of the patient should be made considering the general state of the patient and the specific characteristics of their presenting condition. The choice of system, i.e. garment and treatment regime, is to be recommended by the medical practitioner for the patient.

Training and education of the patient in the use and understanding of the system will help to ensure compliance.

- Indications**
- Lymphedema - primary
- secondary;
 - Oedema - dependent
- traumatic
- secondary to stroke;
 - Chronic Venous Insufficiency

- Cautions**
1. Proper application and connection to the pump is essential.
 2. Garments should be removed if the patient experiences tingling, numbness or pain.

Contraindications

POWERPRESS unit should NOT be used in the following conditions:

1. Severe arteriosclerosis or other ischemic vascular diseases.
2. Known or suspected acute deep vein thrombosis.
3. Severe congestive cardiac failure.
4. Any local condition in which garments would interfere, for example:
 - Gangrene
 - Untreated, infected leg wounds
 - Recent skin graft
 - Dermatitis


3. Clinical Treatment Guide

An initial pressure of 40 mmHg (30 mmHg for management of lymphedema) is suggested at the commencement of treatment. It may be necessary to start at a lower level of pressure, dependent on the patient's tolerance.


The pressure can be gradually increased over time, until the required pressure is reached. The upper treatment pressure range is generally 60-70 mmHg.

A single treatment session is usually 20-60 minutes. The above settings and timings are guidelines, and should not be used as a substitute for clinical judgement and experience.

4. Garments type & size

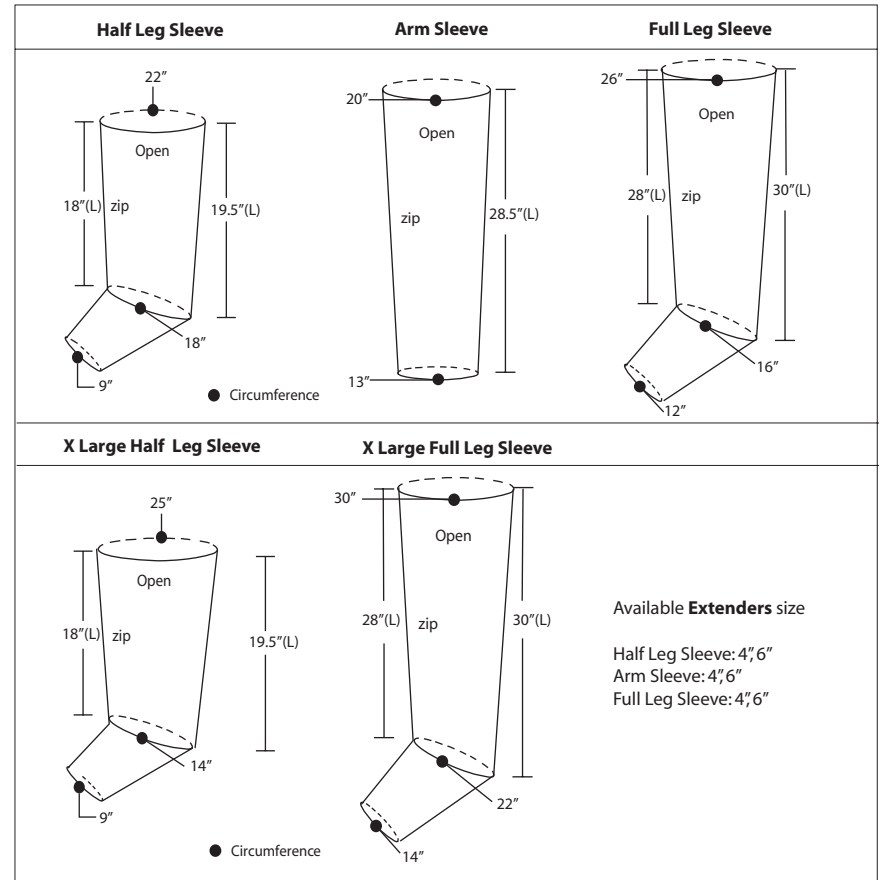

5. Pump Description

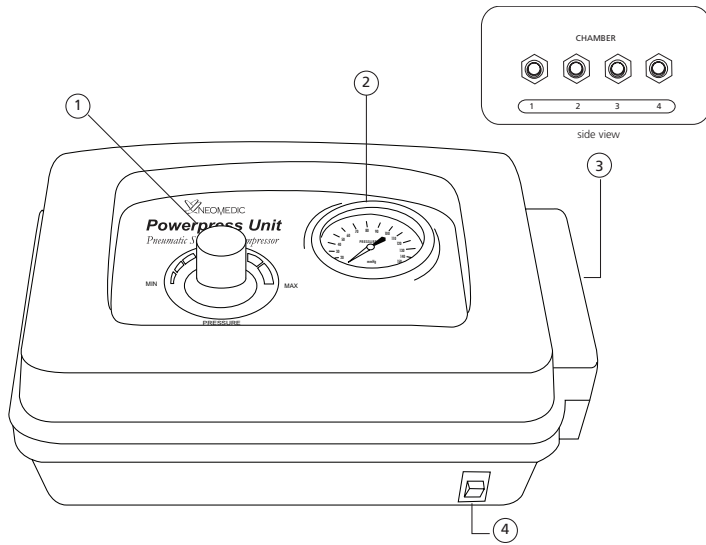

- 1 Main Pressure Controller Knob (Push to Lock, Pull to release)
- 2 Pressure Gauge (0 ~ 160mmHg)
- 3 Air Tubing Hose Connector
- 4 Power Switch

Operation: The pump should be placed securely on a flat surface. Before starting the pump ensure that the garments are properly applied, the zippers are secured and the garment connecting tubes are attached to the pump outlet ports.

How to SET UP Pressure?

• Model# P1000

1. Turn on Power Switch
2. Wait until deflation time

During Deflation Time; Pressure Gauge does not move
Air does not inflate sleeves
Air in the sleeves comes out
Air does not come out from connection port

3. Turn Pressure Knob quickly and set to desired pressure
4. Connect Tubing Hose and wear sleeves.

During usage of Pump : Wait until deflation time to set desired pressure

To Remove the Garment: Switch off the pump, disconnect the tubing from the pump by removing the tube connectors.

6. Warranty

All Powerpress Unit shall conform to applicable specifications in effect from the invoice date to the end of the Warranty Period, and Powerpress Unit reserves the right to change such specifications at any time with or without notice. The Warranty Period for Powerpress Unit products shall be as follows, calculated from the date of invoice:

- The Powerpress Unit pump is guaranteed for 12 months
- The powerpress Unit garments are guaranteed for 6 months

7. Safety Warnings

- Electrical equipment may be hazardous if misused. The pump's rear case should only be removed by authorized technical personnel.
- Do not use the pump in the presence of flammable gases such as anesthetic agents.
- Make sure that the main power cable is positioned to avoid causing a trip or other hazard, and is clear of moving bed mechanisms or other possible entrapment areas.

8. Caution

Electromagnetic compatibility (EMC). This product complies with the requirements of applicable EMC Standards. The use of accessories not specified by the manufacturer may result in increased emissions by, or decreased immunity of, the equipment, affecting its performance.

9. Troubleshooting

If you should encounter a problem, please follow the fault finding guide below, if the fault cannot be rectified, please refer to Service.

Fault	Check	Remedy
Pump does not operate.	Is power switch on? Is power cord plugged in correctly?	Check switch. Check connections.
Pump operates but garments will not inflate. None of the above.	Blockage in garment supply tube. Garment not correctly fitted to pump. Pressure control set too low. Air leak in garment.	Ensure that the tube airway is clear. Check connections. Increase pressure control. Check garment. Replace if defective. <i>Hint - Reduced pressure level indicates garment or connector leak</i>
None of the above.	Call Service	

10. Technical Description

Model No:	P1000
Supply Voltage:	120 V
Supply Frequency:	60 Hz
Electrical Rating:	14VA
Fuse Rating:	F500mAH250V
Size:	Length: 11.8" (300mm)
	Width: 8.3" (210mm)
	Height: 5.1" (130mm)
	Weight: 4.5lbs (2kg)
Case Material:	ABS Plastic
Mode of Operation:	Continuous